

### Safe and Efficient Cryogenic Grinding of Food Samples

Author details: Dr Tanja Butt, Retsch GmbH, t.butt@retsch.com

Most sample materials can be ground to the required analytical fineness at room temperature. However, there are limits, for example when even a small temperature increase affects the sample in a negative way; or when the material is very elastic and will only be deformed. Moreover, food samples which are fatty or sticky may block the mill. Therefore, cryogenic grinding is the best way to pulverise food samples like cheese, raisins, wine gum or marzipan which simply clump together when ground at room temperature.

Another important aspect is the preservation of volatile sample components. The heat which is generated during the grinding process would cause volatiles like alcohol or residues of softeners from plastic wrappings to escape. This effect is prevented by using grinding aids like liquid nitrogen (LN<sub>2</sub>; -196°C) or dry ice (solid CO<sub>2</sub>; -78°C) which also embrittle the sample and make it break more easily. In the following, the special requirements for cryogenic grinding in different mills will be discussed as well as which other aspects need to be taken into consideration (Table 1).

Table 1. Overview of mills suitable for cryogenic grinding

Mill	Feed size and max. feed quantity *	Remark
Mixer mill	<8 mm 2 x 20 ml	<ul style="list-style-type: none"> <li>Sample is placed in leak-free grinding jar of steel or PTFE and embrittled before grinding, LN<sub>2</sub> preferred over dry ice</li> <li>Intermediate cooling may be required</li> </ul>
CryoMill	<8 mm 1 x 20 ml	<ul style="list-style-type: none"> <li>Continuous grinding at -196 °C with LN<sub>2</sub></li> <li>User comes at no point in contact with LN<sub>2</sub></li> <li>Zirconium oxide grinding jar available for cryogenic grinding</li> </ul>
Knife mill	<40 mm 2000 ml	<ul style="list-style-type: none"> <li>Embrittlement with dry ice</li> <li>Dry ice cools sample during grinding</li> <li>Use of full metal knife, grinding container of stainless steel and specific lid mandatory</li> </ul>
Ultra centrifugal mill	<10 mm 4000 ml	<ul style="list-style-type: none"> <li>Embrittlement with dry ice or LN<sub>2</sub></li> <li>Dry ice preferred if sample material is &lt; 1 mm or has low thermal capacity</li> <li>Use of cyclone mandatory</li> </ul>
Cutting mill	<80 mm 4000 ml	<ul style="list-style-type: none"> <li>Cryogenic grinding with dry ice or LN<sub>2</sub></li> <li>Use of 6-disc rotor and cyclone mandatory</li> <li>Bottom sieves 2 – 20 mm suitable</li> </ul>

\*both depending on sample material

#### Small Sample Volumes and Feed Sizes in the Mixer Mill MM 400 and the CryoMill

Sample volumes like a few gummy bears, some strips of chewing gum, a small piece of meat or small amounts of fatty spices are best homogenised in the MM 400. This ball mill is perfectly suited for homogenising sample volumes up to 2 x 20 ml in less than 1-2 minutes. It is important to fill the jar first with the grinding ball(s) and with the sample and close it tightly before embrittling. Care must be taken that no LN<sub>2</sub> is enclosed in the



Figure 1. The CryoMill offers the advantage of continuous cooling of the grinding jar with LN<sub>2</sub>

grinding jars because the evaporation of LN<sub>2</sub> would result in a considerable pressure increase inside the grinding jar. The closed grinding jars, and thus the sample, are embrittled in a LN<sub>2</sub> bath for 2-3 minutes. Suitable grinding jars for cryogenic grinding are made of steel or PTFE; it is not recommended to use jars made of different materials (e. g. steel jar with lining of zirconium oxide). This is important, as these may react differently to extreme temperatures of -196°C which may lead to damages of the jar. Single-use vials of 1.5, 2 and 5 ml are also available for cryogenic grinding when it comes to sample amounts below 0.7 ml. Due to the high energy input and the resulting frictional heat, the grinding process should not take longer than 2 minutes to prevent the sample from warming up and to preserve its breaking properties. If longer grinding times are required, these should be interrupted by intermediate cooling of the closed grinding jars in the MM 400.

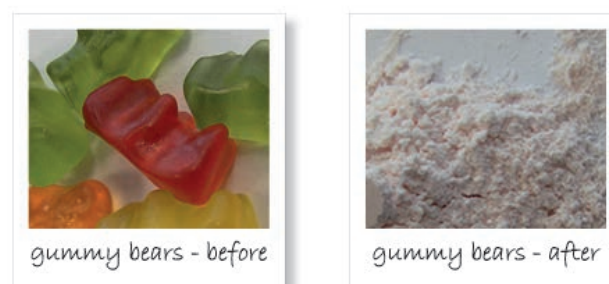


Figure 2. Gummy bears before and after cryogenic grinding in the Mixer Mill MM 400

Cryogenic grinding in the CryoMill offers the advantage of continuous cooling of the grinding jar with LN<sub>2</sub>, thereby reducing the temperature of jar and sample to -196°C within minutes. This consistent temperature is guaranteed even for long grinding times without the need for intermediate cooling breaks. An automatic pre-cooling function ensures that the grinding process does not start before a temperature of -196°C is reached and maintained. Moreover, operation is particularly safe as the user comes at no point into

contact with LN<sub>2</sub>. For heavy-metal-free grinding a zirconium oxide grinding jar should be used. Further suitable materials are stainless steel or single use vials (1.5 or 2 ml). A few pieces of liquorice, one praline with liquid filling or some beans of green coffee are typical samples for the CryoMill.

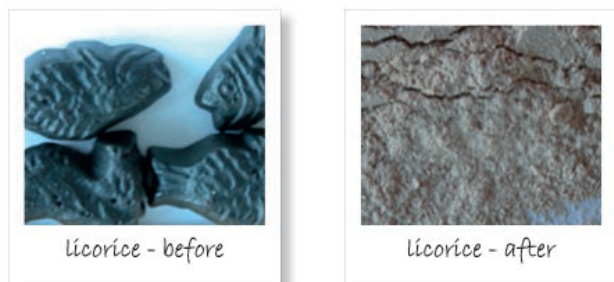


Figure 3: Licorice before and after grinding in the CryoMill

### Medium Sample Volumes with Medium Initial Sample Size in the Knife Mill GM 300

Medium sample volumes of up to 2 l with a feed size not bigger than 40 mm, such as 500 g wine gum, 250 g grapes, 400 g pure bacon or 800 g raisin, can be homogenised perfectly in the GM 300 by using dry ice snow as grinding aid. The use of LN<sub>2</sub> is not recommended as the mill is not designed for temperatures as low as -196°C. The sample is mixed with dry ice in a ratio of 1:2; after a few minutes, it is thoroughly cooled, and the grinding process starts. The dry ice keeps the sample cool all the time. Care should be taken not to use any plastic accessories when carrying out cryogenic grinding in the knife mills as these could be damaged during the process. Suitable accessories include a grinding container of stainless steel, a full metal knife and a lid with aperture to allow evaporation of the gaseous carbon dioxide.



Figure 4: Bacon before and after grinding in the Knife Mill GRINDMIX GM 300

### Large Sample Volumes with Small Initial Sample Size in the Ultra Centrifugal Mill ZM 200

The Ultra Centrifugal Mill ZM 200 accepts large sample volumes up to 4 l with a feed size < 10 mm, such as 100 g cereals, 150 g onions or 100 g dried apple pieces. The sample is directly immersed into a container filled with LN<sub>2</sub> before being continuously but slowly fed to the hopper of the mill with a steel spoon. When using dry ice as grinding aid, this needs to be mixed with the sample (1 part sample, 2 parts dry ice) and the entire mixture is then pulverised in the mill. Using a cassette in combination with a cyclone is recommended for cryogenic grinding to ensure that the evaporating cooling agent is completely discharged during the grinding process.



Figure 5: Ultra Centrifugal Mill ZM 200

### Large Sample Volumes with Large Feed Sizes in the Cutting Mill SM 300

Large sample volumes up to 4 l with feed sizes up to 80 mm, like a block of 100 g chocolate, 1 kg trout (whole fish) or 20 kg potatoes are best processed in the Cutting Mill SM 300. The use of both LN<sub>2</sub> and dry ice is possible. The embrittled sample material is rather hard, therefore the use of the 6-disc rotor is recommended as it works rather like a shredder. It is also suitable to cut heterogeneous samples such as frozen chicken parts including bones. The SM 300 is designed for pre-crushing bigger sample pieces <4 mm. Pulverisation of the samples then follows in one of the other mills described above.

### Conclusion

Some foodstuff needs to be pulverised under cryogenic conditions, i. e. by using dry ice or liquid nitrogen as grinding aid, to obtain a sample which is suitable for subsequent analysis. Retsch offers a variety of laboratory mills designed for gentle and efficient cold grinding of food samples which ensure the whole process is time and cost effective. A wide range of accessories helps to make the grinding process safe and user-friendly.

